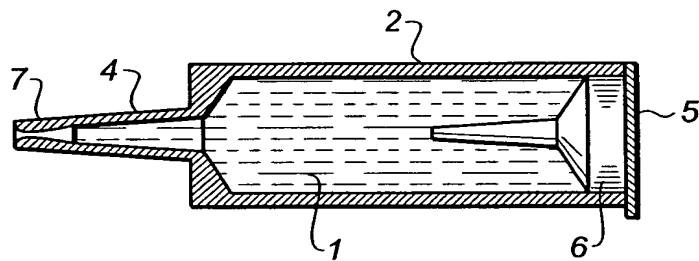
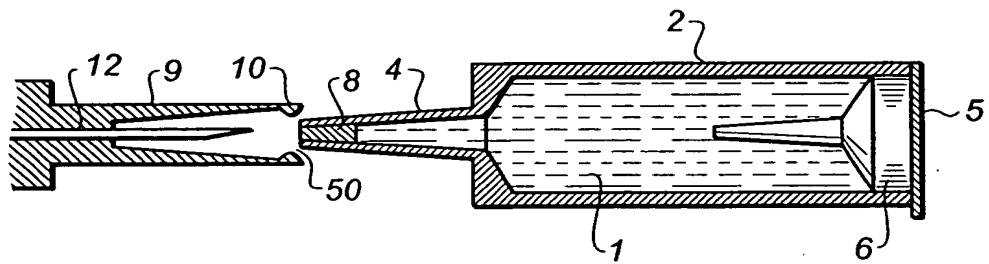


**FIG. 1**



**FIG. 2**



**FIG. 3**

FIG. 4 is a cross-sectional view of the device in a first position, and FIG. 5 is a cross-sectional view of the device in a second position.

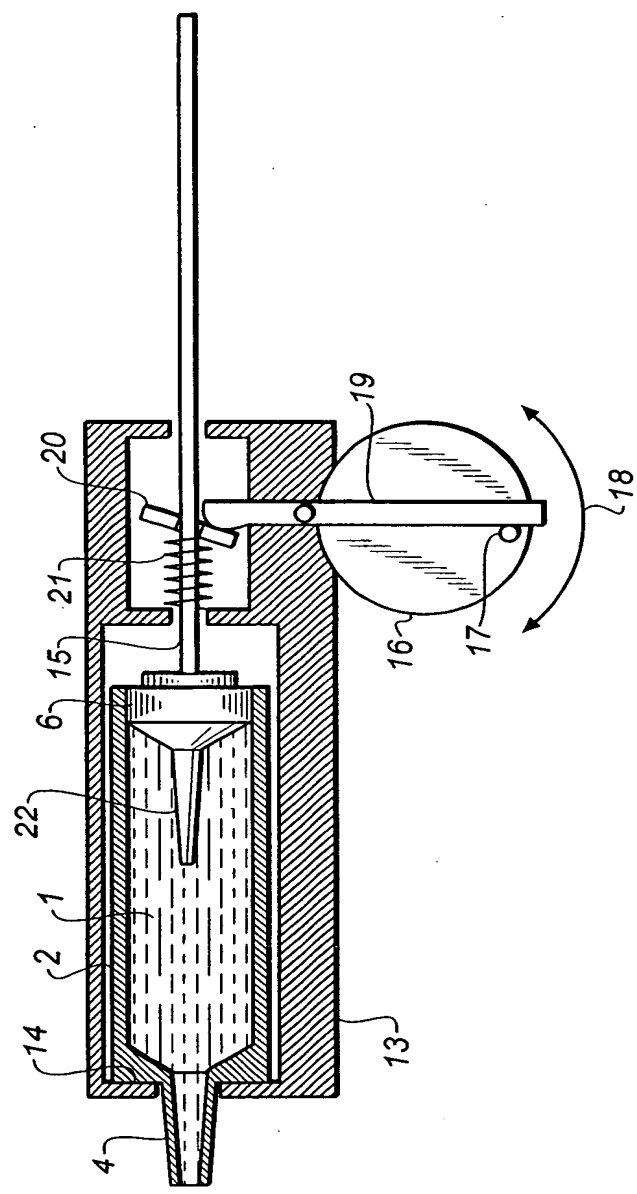


FIG. 4

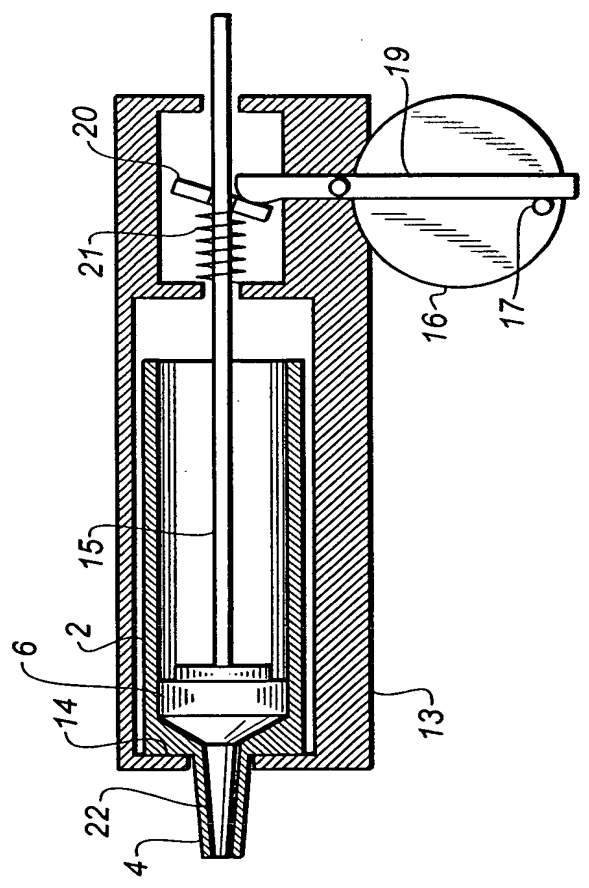


FIG. 5

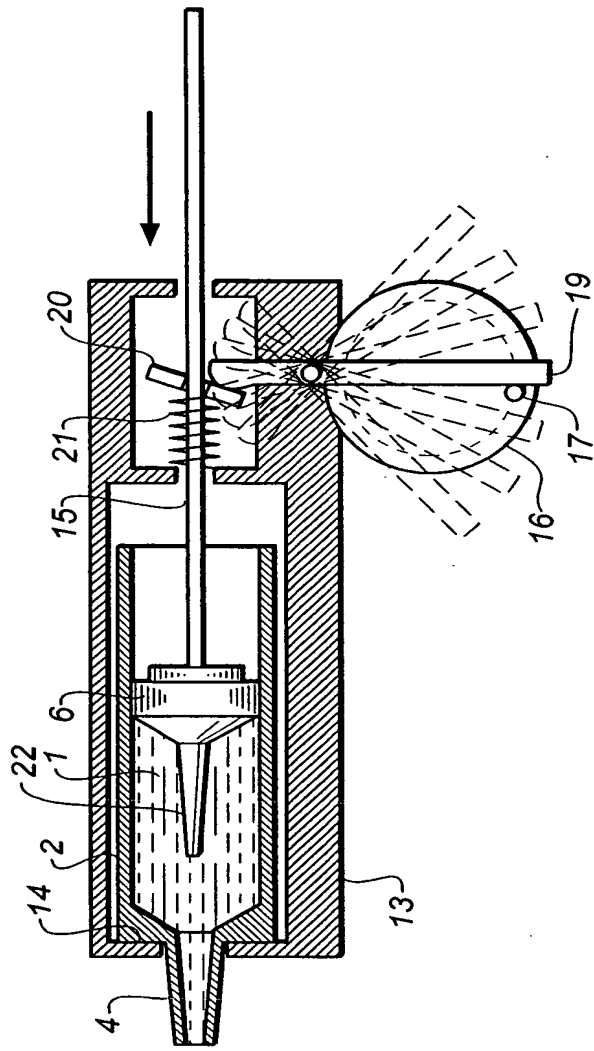


FIG. 6

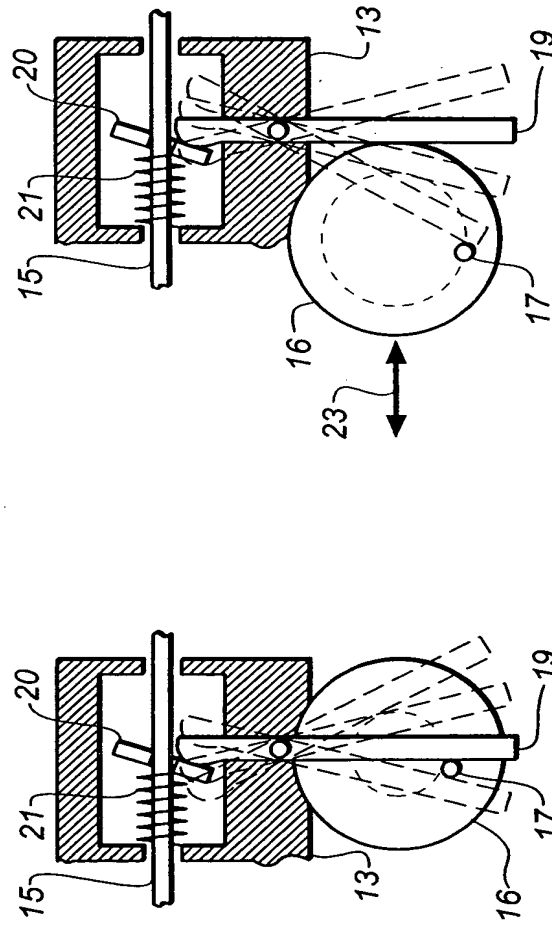


FIG. 7B

FIG. 7A

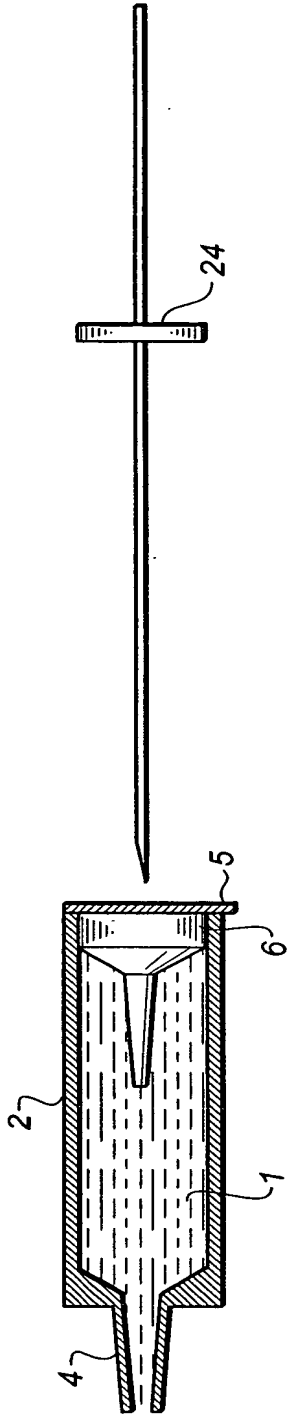


FIG. 8A

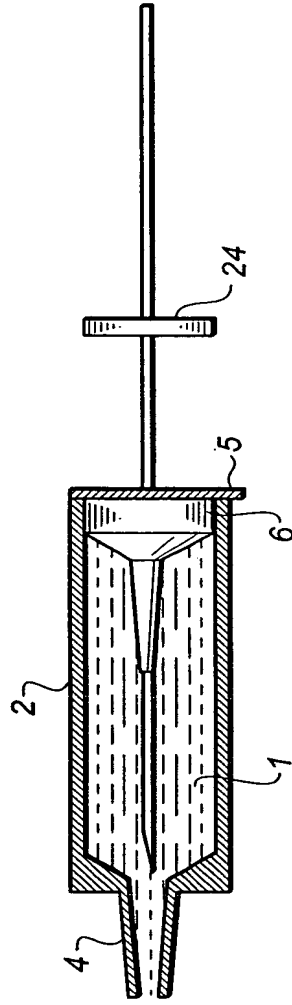


FIG. 8B

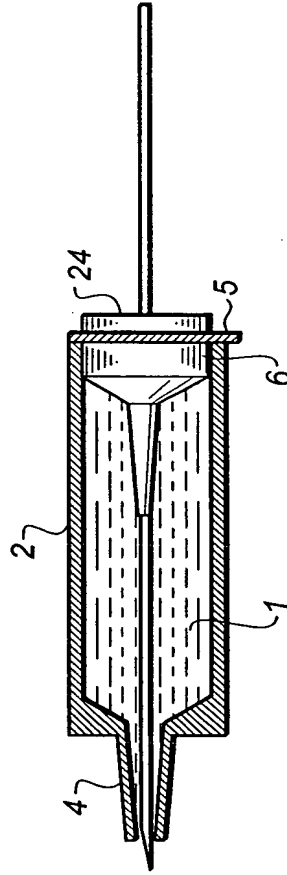


FIG. 8C

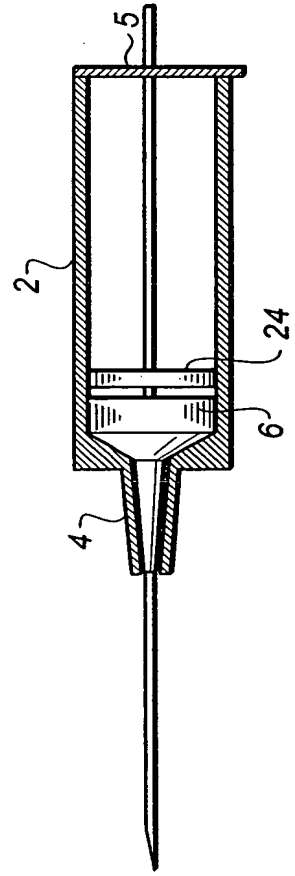


FIG. 8D

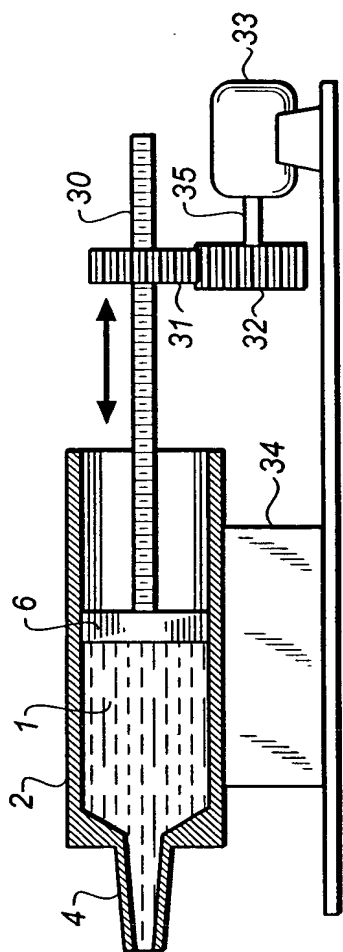


FIG. 9

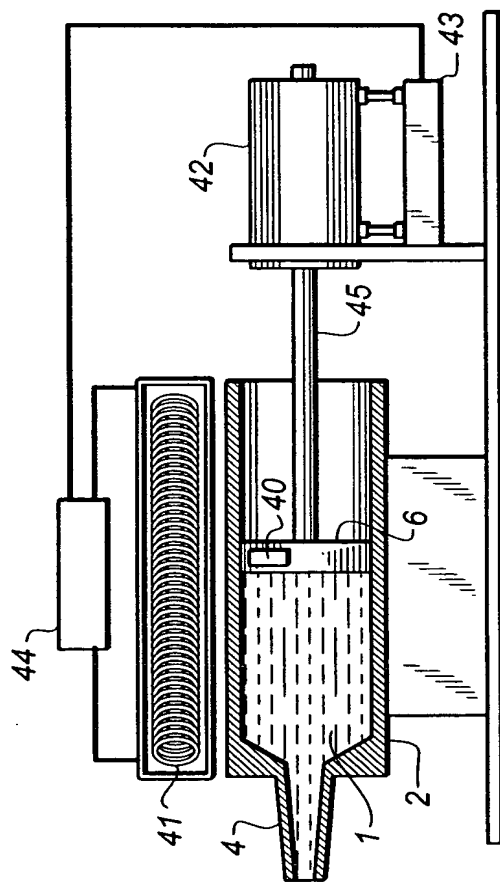


FIG. 10